



Standard Practice for Design, Manufacture and Material Grouping Classification of Wire Image Quality Indicators (IQI) Used for Radiology¹

This standard is issued under the fixed designation E 747; the number immediately following the designation indicates the year of original adoption or, in the case of revision, the year of last revision. A number in parentheses indicates the year of last reapproval. A superscript epsilon (ϵ) indicates an editorial change since the last revision or reapproval.

1. Scope

1.1 This practice² covers the design, material grouping classification, and manufacture of wire image quality indicators (IQI) used to indicate the quality of radiologic images.

1.2 This practice is applicable to X-ray and gamma-ray radiology.

1.3 This practice covers the use of wire penetrameters as the controlling image quality indicator for the material thickness range from 6.4 to 152 mm (0.25 to 6.0 in.).

1.4 The values stated in inch-pound units are to be regarded as standard.

1.5 *This standard does not purport to address all of the safety concerns, if any, associated with its use. It is the responsibility of the user of this standard to establish appropriate safety and health practices and determine the applicability of regulatory limitations prior to use.*

2. Referenced Documents

2.1 ASTM Standards:

B 139 Specification for Phosphor Bronze Rod, Bar, and Shapes³

B 150 Specification for Aluminum Bronze Rod, Bar, and Shapes³

B 161 Specification for Nickel Seamless Pipe and Tube⁴

B 164 Specification for Nickel-Copper Alloy Rod, Bar, and Wire⁴

B 166 Specification for Nickel-Chromium-Iron Alloys (UNS N06600, N06601, and N06690) and Nickel-Chromium-Cobalt-Molybdenum Alloy (UNS N06617) Rod, Bar, and Wire⁴

E 1025 Practice for Design, Manufacture, and Material Grouping Classification of Hole-Type Image Quality Indicators (IQI) Used for Radiology⁵

E 1316 Terminology for Nondestructive Examinations⁵

¹ This practice is under the jurisdiction of ASTM Committee E-7 on Nondestructive Testing and is the direct responsibility of Subcommittee E07.01 on Radiographic Practice and Penetrameters.

Current edition approved July 10, 1997. Published November 1997. Originally published as E 747 – 80. Last previous edition E 747 – 94.

² For ASME Boiler and Pressure Vessel Code applications see related Practice SE-747 in Section II of that Code.

³ *Annual Book of ASTM Standards*, Vol 02.01.

⁴ *Annual Book of ASTM Standards*, Vol 02.04.

⁵ *Annual Book of ASTM Standards*, Vol 03.03.

3. Terminology

3.1 *Definitions*—The definitions of terms in Terminology E 1316, Section D, relating to gamma and x-radiology, shall apply to the terms used in this practice.

4. Wire IQI Requirements

4.1 The quality of all levels of examination shall be determined by a set of wires conforming to the following requirements:

4.1.1 Wires shall be fabricated from materials or alloys identified or listed in accordance with 7.2. Other materials may be used in accordance with 7.3.

TABLE 1 Wire IQI Sizes and Wire Identity Numbers

SET A		SET B	
Wire Diameter in. (mm)	Wire Identity	Wire Diameter in. (mm)	Wire Identity
0.0032 (0.08) ⁴	1	0.010 (0.25)	6
0.004 (0.1)	2	0.013 (0.33)	7
0.005 (0.13)	3	0.016 (0.4)	8
0.0063 (0.16)	4	0.020 (0.51)	9
0.008 (0.2)	5	0.025 (0.64)	10
0.010 (0.25)	6	0.032 (0.81)	11
SET C		SET D	
Wire Diameter in. (mm)	Wire Identity	Wire Diameter in. (mm)	Wire Identity
0.032 (0.81)	11	0.10 (2.5)	16
0.040 h(1.02)	12	0.126 (3.2)	17
0.050 (1.27)	13	0.160 (4.06)	18
0.063 (1.6)	14	0.20 (5.1)	19
0.080 (2.03)	15	0.25 (6.4)	20
0.100 (2.5)	16	0.32 (8)	21

⁴ The 0.0032 wire may be used to establish a special quality level as agreed upon between the purchaser and the supplier.

TABLE 2 Wire Diameter Tolerances, (mm)

Wire Diameter (d), mm	Tolerance, mm
0.000 < d ≤ 0.125	±0.0025
0.125 < d ≤ 0.25	±0.005
0.25 < d ≤ 0.5	±0.01
0.50 < d ≤ 1.6	±0.02
1.6 < d ≤ 4	±0.03
4.0 < d ≤ 8	±0.05

4.1.2 The IQI consists of sets of wires arranged in order of increasing diameter. The diameter sizes specified in Table 1 are

TABLE 3 Wire Diameter Tolerances, (in.)

Wire Diameter (d), in.	Tolerance, in.
0.000 < d ≤ 0.005	±0.0001
0.005 < d ≤ 0.010	±0.0002
0.010 < d ≤ 0.020	±0.0004
0.020 < d ≤ 0.063	±0.0008
0.063 < d ≤ 0.160	±0.0012
0.160 < d ≤ 0.320	±0.0020

established from a consecutive series of numbers taken in general from the ISO/R 10 series. The IQI shall be fabricated in accordance with the requirements specified in Figs. 1-8 and Tables 1-3. IQIs previously manufactured to the requirements of Annex A1 may be used as an alternate provided all other requirements of this practice are met.

4.1.3 Image quality indicator (IQI) designs other than those shown in Figs. 1-8 and Annex A1 are permitted by contractual agreement. If an IQI set as listed in Table 1 or Annex A1 is modified in size, it must contain the grade number, set identity, and essential wire. It must also contain two additional wires that are the next size larger and the next size smaller as specified in the applicable set listed in Table 1.

4.1.4 Each set must be identified using letters and numbers made of industrial grade lead or of a material of similar radiographic density. Identification shall be as shown on Figs. 1-8 or Annex A1, unless otherwise specified by contractual agreement.

5. Image Quality Indicator (IQI) Procurement

5.1 When selecting IQI's for procurement, the following factors should be considered:

5.1.1 Determine the alloy group(s) of the material to be examined.

5.1.2 Determine the thickness or thickness range of the material(s) to be examined.

5.1.3 Select the applicable IQI's that represent the required IQI thickness(s) and alloy(s).

6. Image Quality Levels

6.1 The quality level required using wire penetrameters shall be equivalent to the 2-2T level of Practice E 1025 for hole-type IQI's unless a higher or lower quality level is agreed upon between purchaser and supplier. Table 4 provides a list of various hole-type IQI's and the diameter of wires of corresponding equivalent penetrometer sensitivity (EPS) with the applicable 1T, 2T, and 4T holes in the IQI. This table can be used for determining 1T, 2T, and 4T quality levels. Appendix X1 gives the equation for calculating other equivalencies if needed.

6.2 In specifying quality levels, the contract, purchase order, product specification, or drawing should clearly indicate the thickness of material to which the quality level applies. Careful consideration of required quality levels is particularly important.

7. Material Groups

7.1 General:

7.1.1 Materials have been designated in eight groups based on their radiographic absorption characteristics: groups 03, 02, and 01 for light metals and groups 1 through 5 for heavy metals.

7.1.2 The light metal groups, magnesium (Mg), aluminum (Al), and titanium (Ti) are identified 03, 02, and 01 respectively, for their predominant alloying constituent. The materials are listed in order of increasing radiation absorption.

7.1.3 The heavy metal groups, steel, copper-base, nickel-base, and kindred alloys are identified 1 through 5. The materials increase in radiation absorption with increasing numerical designation.

7.1.4 Common trade names or alloy designations have been



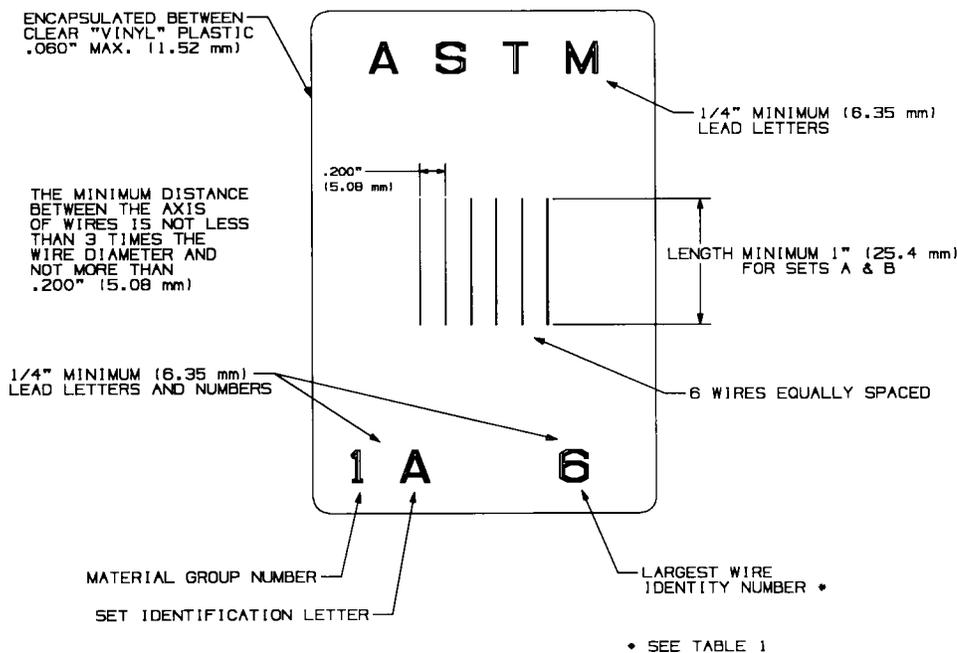


FIG. 1 Set A/Alternate 1

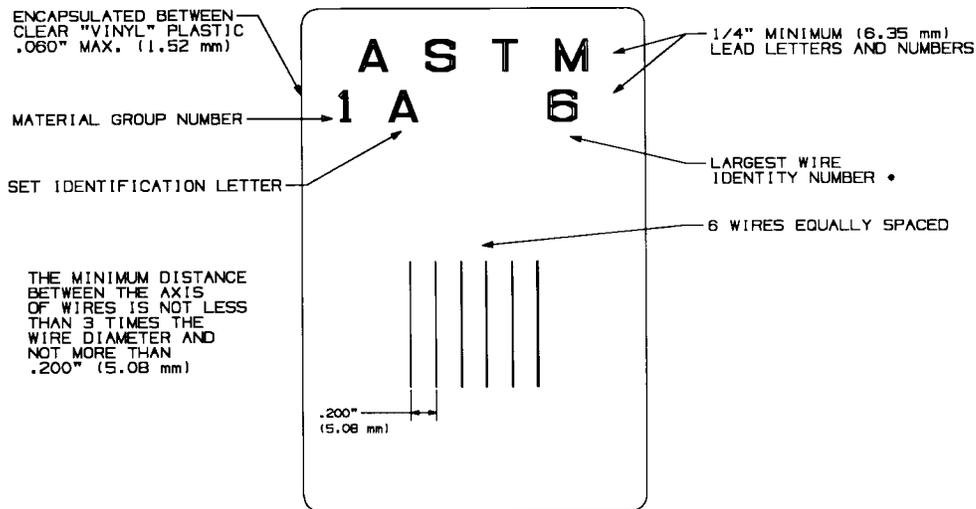

• SEE TABLE 1

FIG. 2 Set A/Alternate 2

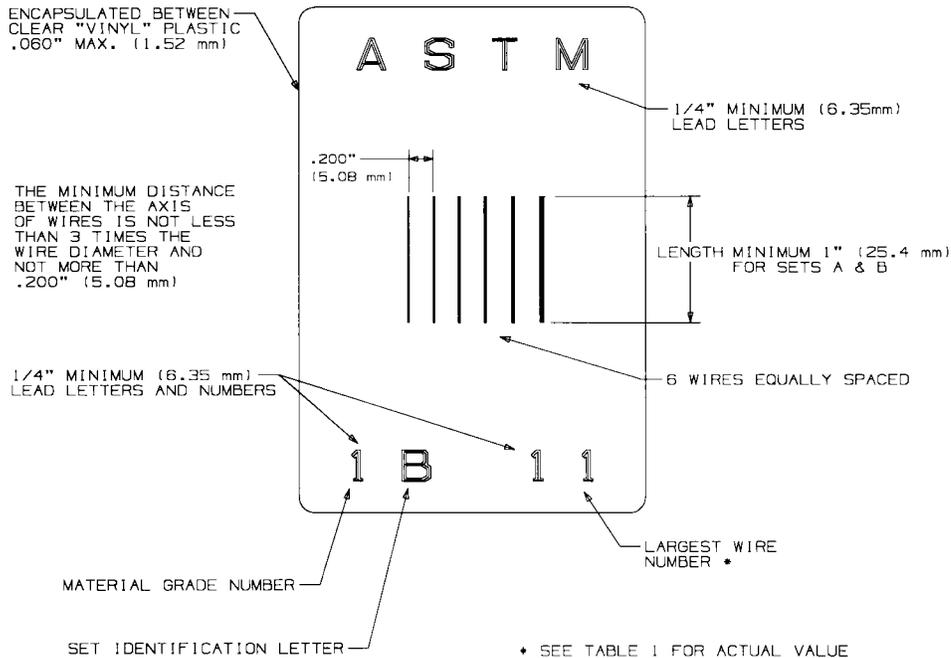

• SEE TABLE 1 FOR ACTUAL VALUE

FIG. 3 Set B/Alternate 1

used for clarification of the pertinent materials.

7.1.5 The materials from which the IQI for the group are to be made are designated in each case and these IQI's are applicable for all materials listed in that group. In addition, any group IQI may be used for any material with a higher group number, provided the applicable quality level is maintained.

7.2 Materials Groups:

7.2.1 Materials Group 01:

7.2.1.1 Image quality indicators (IQI's) shall be made of titanium or titanium shall be the predominant alloying constituent.

7.2.1.2 Use on all alloys of which titanium is the predominant alloying constituent.

7.2.2 Materials Group 02:

7.2.2.1 Image quality indicators (IQI's) shall be made of aluminum or aluminum shall be the predominant alloying constituent.

7.2.2.2 Use on all alloys of which aluminum is the predominant alloying constituent.


7.2.3 Materials Group 03:

7.2.3.1 Image quality indicators (IQI's) shall be made of magnesium or magnesium shall be the predominant alloying constituent.

7.2.3.2 Use on all alloys of which magnesium is the predominant alloying constituent.


7.2.4 Materials Group 1:

7.2.4.1 Image quality indicators (IQI's) shall be made of carbon steel or Type 300 series stainless steel.

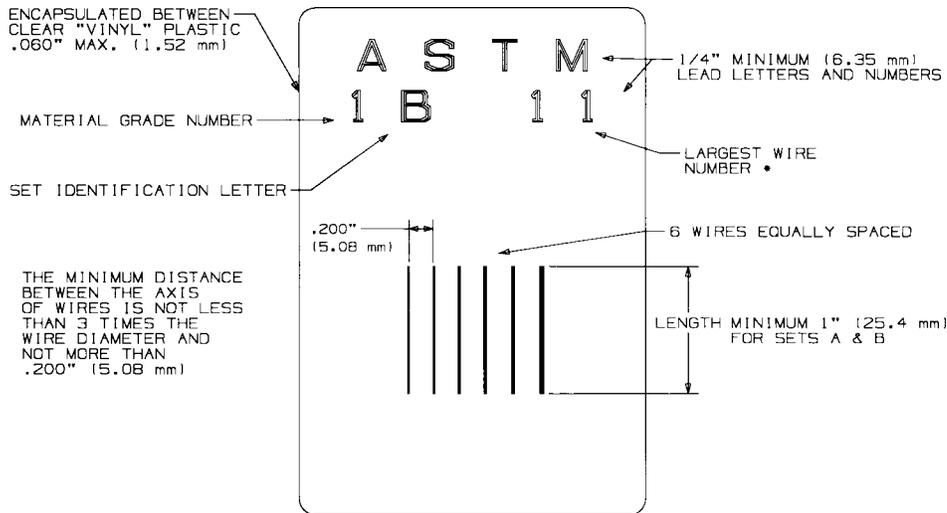

* SEE TABLE 1 FOR ACTUAL VALUE

FIG. 4 Set B/Alternate 2

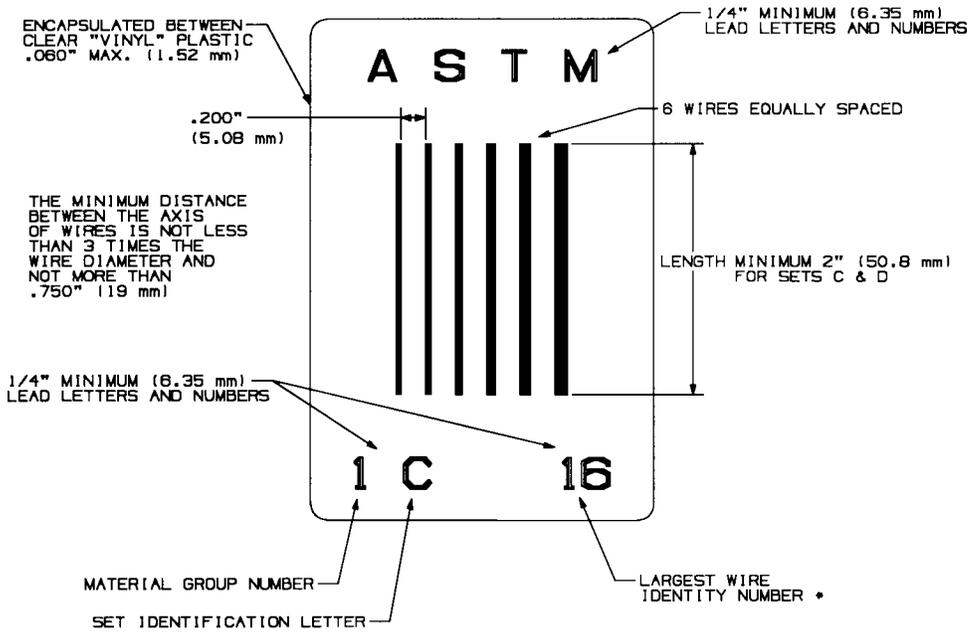

* SEE TABLE 1

FIG. 5 Set C/Alternate 1

7.2.4.2 Use on all carbon steel, low-alloy steels, stainless steels, and manganese-nickel-aluminum bronze (Superston).⁶

7.2.5 *Materials Group 2:*

7.2.5.1 Image quality indicators (IQI's) shall be made of aluminum bronze (Alloy No. 623 of Specification B 150) or equivalent, or nickel-aluminum bronze (Alloy No. 630 of Specification B 150) or equivalent.

7.2.5.2 Use on all aluminum bronzes and all nickel-aluminum bronzes.

7.2.6 *Materials Group 3:*

7.2.6.1 Image quality indicators (IQI's) shall be made of nickel-chromium-iron alloy (UNS No. N06600) (Inconel).⁷ (See Specification B 166).

7.2.6.2 Use on nickel-chromium-iron alloy and 18 % nickel-maraging steel.

7.2.7 *Materials Group 4:*

7.2.7.1 Image quality indicators (IQI's) shall be made of

⁶ Superston is a registered trademark of Superston Corp., Jersey City, NJ.

⁷ Inconel is a registered trademark of The International Nickel Co., Inc., Huntington, WV 25720.

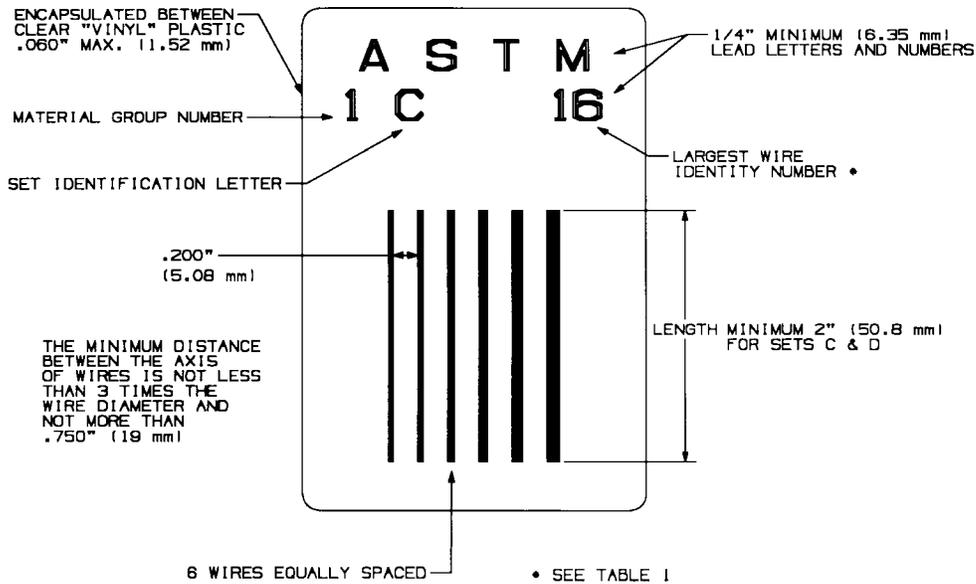


FIG. 6 Set C/Alternate 2

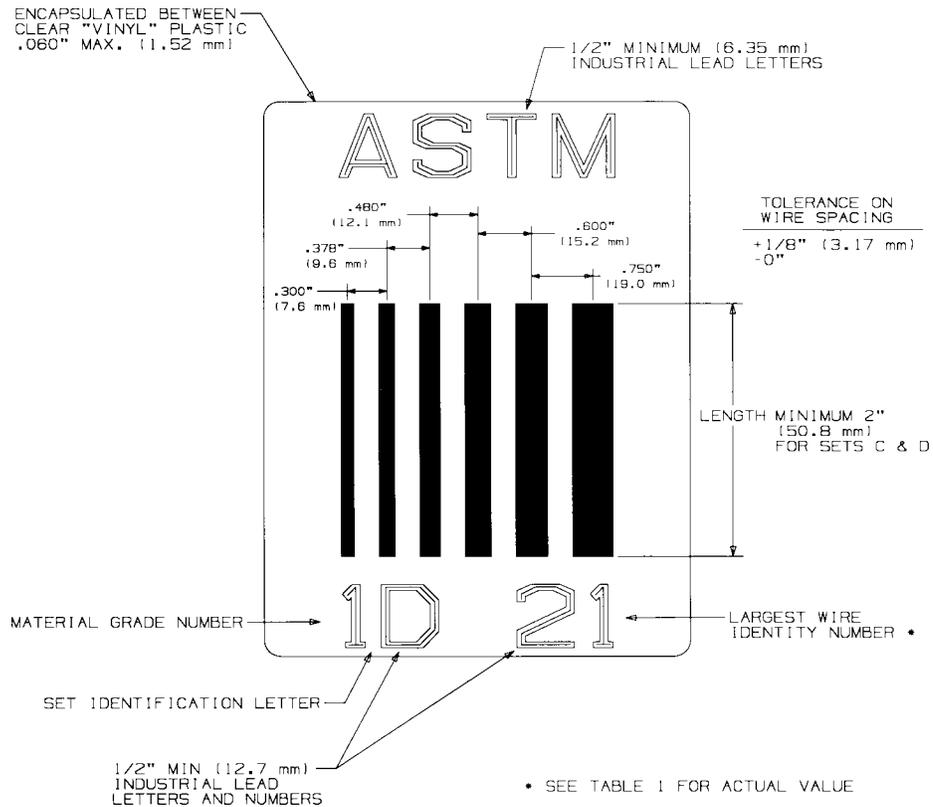


FIG. 7 Set D/Alternate 1

70 to 30 nickel-copper alloy (Monel)⁸ (Class A or B of Specification B 164) or equivalent, or 70 to 30 copper-nickel alloy (Alloy G of Specification B 161) or equivalent.

7.2.7.2 Use on nickel, copper, all nickel-copper series, and copper-nickel series of alloys, and all brasses (copper-zinc


alloys). Group 4 IQI's may include the leaded brasses since leaded brass increases in attenuation with increase in lead content. This would be equivalent to using a lower group IQI.

7.2.8 Materials Group 5:

7.2.8.1 Image quality indicators (IQI's) shall be made of tin bronze (Alloy D of Specification B 139).

7.2.8.2 Use on tin bronzes including gun-metal and valve bronze, or leaded-tin bronze of higher lead content than valve

⁸ Monel is a registered trademark of The International Nickel Co., Inc., Huntington, WV 25720.

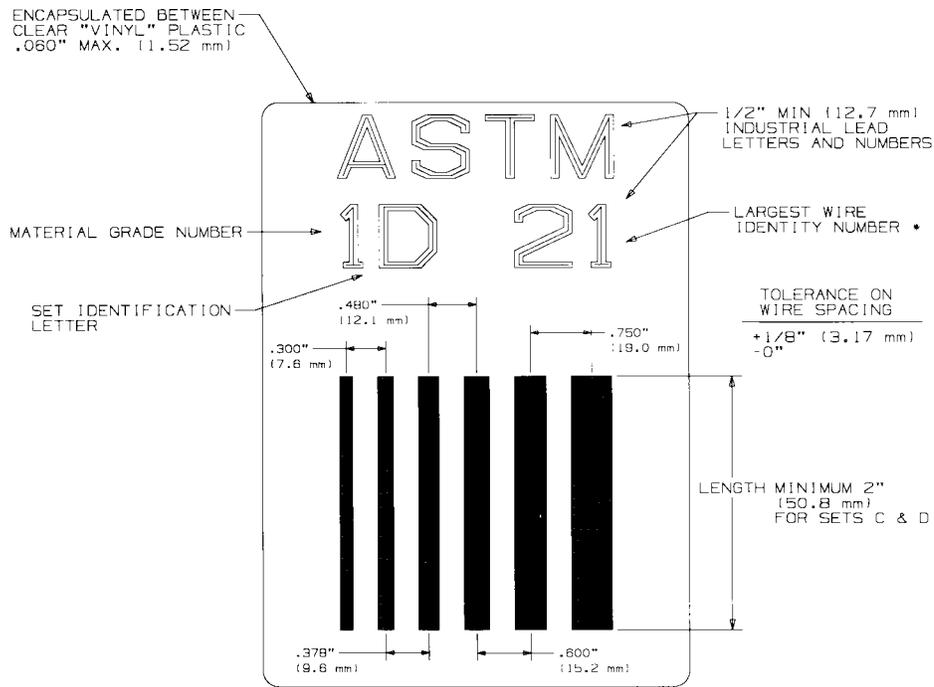

* SEE TABLE 1 FOR ACTUAL VALUE

FIG. 8 Set D/Alternate 2

TABLE 4 Wire Sizes Equivalent to Corresponding 1T, 2T, and 4T Holes in Various Hole Type Plaques

Plaque Thickness, in. (mm)	Plaque IQI Identification Number	Diameter of wire with EPS of hole in plaque, in. (mm)		
		1T	2T	4T
0.005 (0.13)	5		0.0038 (0.09)	0.006 (0.15)
0.006 (0.16)	6		0.004 (0.10)	0.0067 (0.18)
0.008 (0.20)	8	0.0032 (0.08)	0.005 (0.13)	0.008 (0.20)
0.009 (0.23)	9	0.0035 (0.09)	0.0056 (0.14)	0.009 (0.23)
0.010 (0.25)	10	0.004 (0.10)	0.006 (0.15)	0.010 (0.25)
0.012 (0.30)	12	0.005 (0.13)	0.008 (0.20)	0.012 (0.28)
0.015 (0.38)	15	0.0065 (0.16)	0.010 (0.25)	0.016 (0.41)
0.017 (0.43)	17	0.0076 (0.19)	0.012 (0.28)	0.020 (0.51)
0.020 (0.51)	20	0.010 (0.25)	0.015 (0.38)	0.025 (0.63)
0.025 (0.64)	25	0.013 (0.33)	0.020 (0.51)	0.032 (0.81)
0.030 (0.76)	30	0.016 (0.41)	0.025 (0.63)	0.040 (1.02)
0.035 (0.89)	35	0.020 (0.51)	0.032 (0.81)	0.050 (1.27)
0.040 (1.02)	40	0.025 (0.63)	0.040 (0.02)	0.063 (1.57)
0.050 (1.27)	50	0.032 (0.81)	0.050 (1.27)	0.080 (2.03)
0.060 (1.52)	60	0.040 (1.02)	0.063 (1.57)	0.100 (2.54)
0.070 (1.78)	70	0.050 (1.27)	0.080 (2.03)	0.126 (3.20)
0.080 (2.03)	80	0.063 (1.57)	0.100 (2.54)	0.160 (4.06)
0.100 (2.5)	100	0.080 (2.03)	0.126 (3.20)	0.200 (5.08)
0.120 (3.05)	120	0.100 (2.54)	0.160 (4.06)	0.250 (6.35)
0.140 (3.56)	140	0.126 (3.20)	0.200 (5.08)	0.320 (8.13)
0.160 (4.06)	160	0.160 (4.06)	0.250 (6.35)	
0.200 (5.08)	200	0.200 (5.08)	0.320 (8.13)	
0.240 (6.10)	240	0.250 (6.35)		
0.280 (7.11)	280	0.320 (8.13)		

bronze. Group 5 IQI's may include bronze of higher lead content since leaded bronze increases in attenuation with increase in lead content. This would be equivalent to using a lower group IQI.

NOTE 1—In developing the eight listed materials groups, a number of other trade names or other nominal alloy designations were evaluated. For the purpose of making this practice as useful as possible, these materials are listed and categorized, by group, as follows:

(1) Group 2—Haynes Alloy IN-100.⁹

(2) Group 3—Haynes Alloy No. 713C, Hastelloy D¹⁰, G.E. Alloy SEL, Haynes Stellite Alloy No. 21, GMR-235 Alloy, Haynes Alloy No. 93, Inconel X⁷, Inconel 718, and Haynes Stellite Alloy No. S-816.

⁹ All Haynes alloys are registered trademarks of Union Carbide Corp., New York, NY.

¹⁰ All Hastelloys and Haynes Stellite alloys are registered trademarks of the Cabot Corp., Boston, MA.

(3) *Group 4*—Hastelloy Alloy F, Hastelloy Alloy X, and Multimeter Alloy Rene 41.

(4) *Group 5*—Alloys in order of increasing attenuation: Hastelloy Alloy B, Hastelloy Alloy C, Haynes Stellite Alloy No. 31, Thetaloy, Haynes Stellite No. 3, Haynes Alloy No. 25. Image quality indicators (IQI's) of any of these materials are considered applicable for the materials that follow it.

NOTE 2—The committee formulating these recommendations recommend other materials may be added to the materials groups listed as the need arises or as more information is gained, or that additional materials groups may be added.

7.3 Method for Other Materials:

7.3.1 For materials not herein covered, IQI's of the same materials, or any other material, may be used if the following requirements are met. Two blocks of equal thickness, one of the material to be examined (production material) and one of the IQI material, shall be radiographed on one film by one exposure at the lowest energy level to be used for production. Transmission densitometer measurements of the radiographic image of each material shall be made. The density of each image shall be between 2.0 and 4.0. If the image density of the IQI material is within 1.00 to 1.15 times (−0 % to + 15 %) the image density of the production material, IQI's made of that IQI material may be used in radiography of that production

material. The percentage figure is based on the radiographic density of the IQI material.

7.3.2 It shall always be permissible to use IQI's of similar composition as the material being examined.

8. Image Quality Indicator (IQI) Certification

8.1 Documents shall be provided by the IQI manufacturer attesting to the following:

8.1.1 IQI identification alternate, if used.

8.1.2 Material type.

8.1.3 Conformance to specified tolerances for dimensional values.

8.1.4 ASTM standard designation, for example, ASTM E 747—(year designation) used for manufacturing.

9. Precision and Bias

9.1 *Precision and Bias*—No statement is made about the precision or bias for indicating the quality of images since the results merely state whether there is conformance to the criteria for success specified in this practice.

10. Keywords


10.1 density; image quality level; IQI; radiologic; radiology; x-ray and gamma radiation

ANNEX

(Mandatory Information)


A1. ALTERNATE IQI IDENTIFICATION

A1.1 The use of IQI's with identifications as shown on Figs. A1.1-A1.9 and as listed in Table A1.1 is permitted as an acceptable alternate provided all other requirements of Practice E 747 are satisfied.

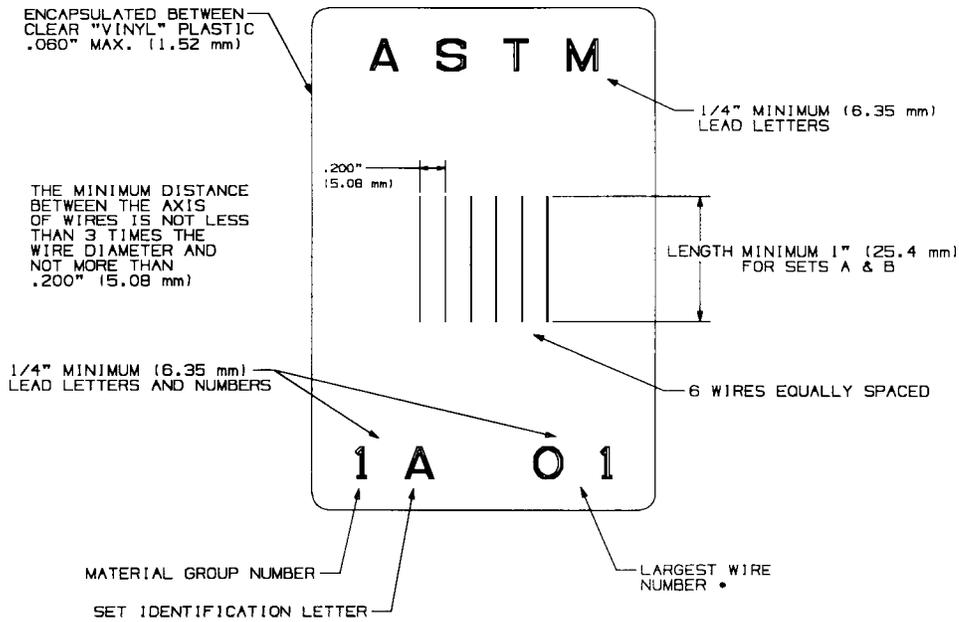


* SEE TABLE 1

FIG. A1.1 Set A/Alternate 1

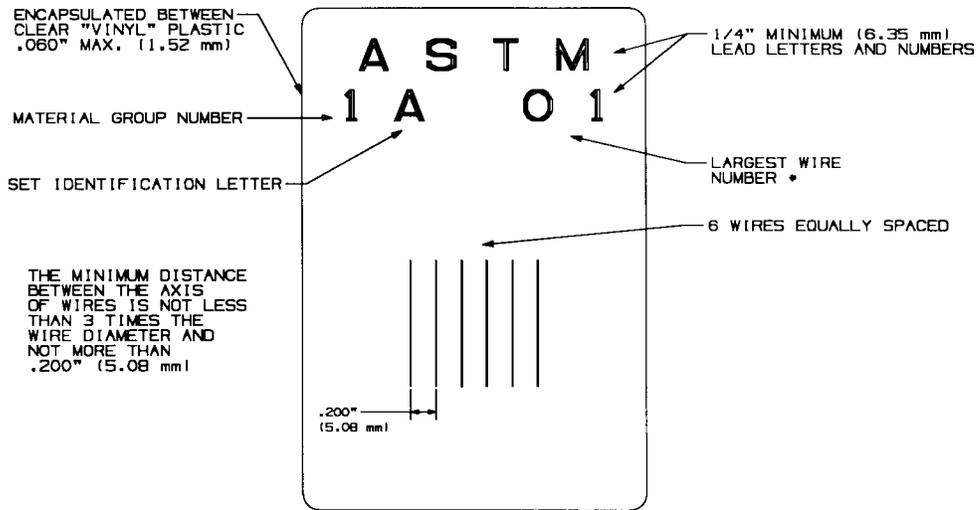


* SEE TABLE 1

FIG. A1.2 Set A/Alternate 2

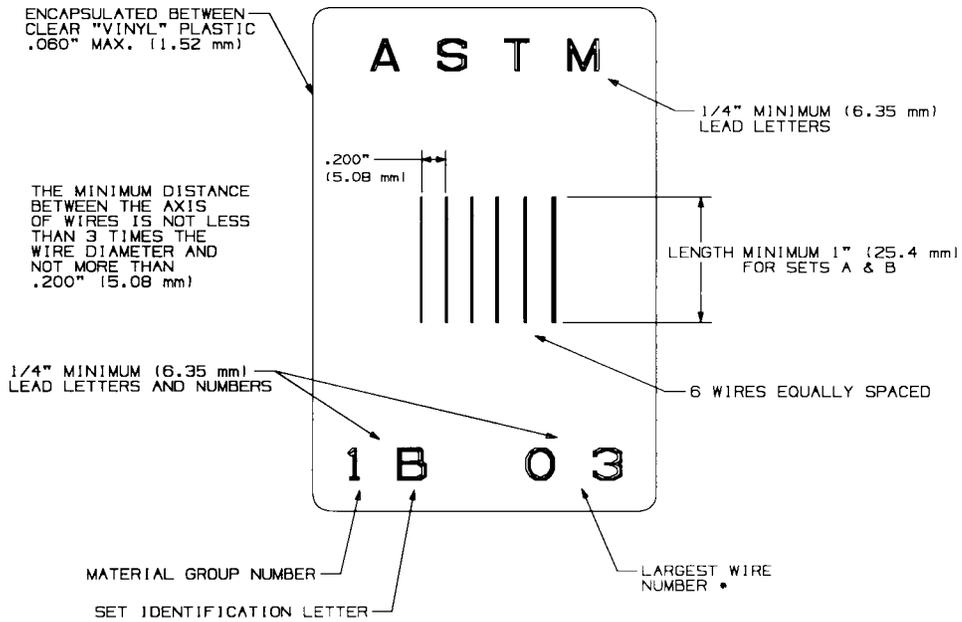

* SEE TABLE 1 FOR ACTUAL VALUE

FIG. A1.3 Set B/Alternate 1

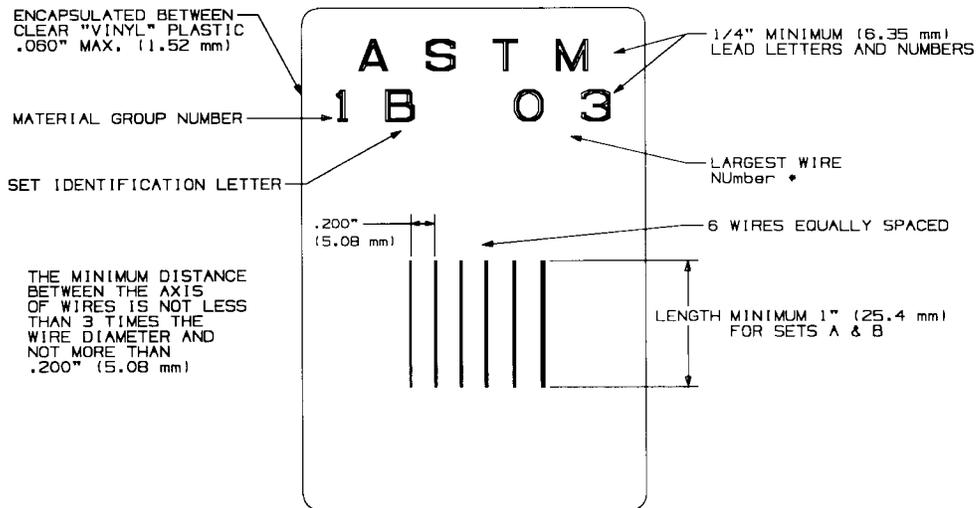

* SEE TABLE 1 FOR ACTUAL VALUE

FIG. A1.4 Set B/Alternate 2

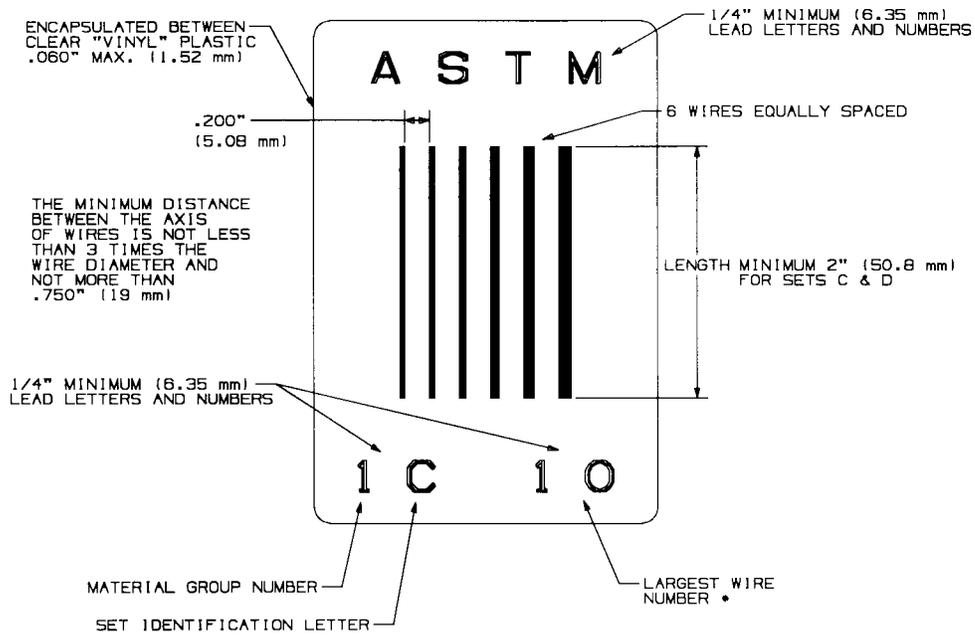


FIG. A1.5 Set C/Alternate 1

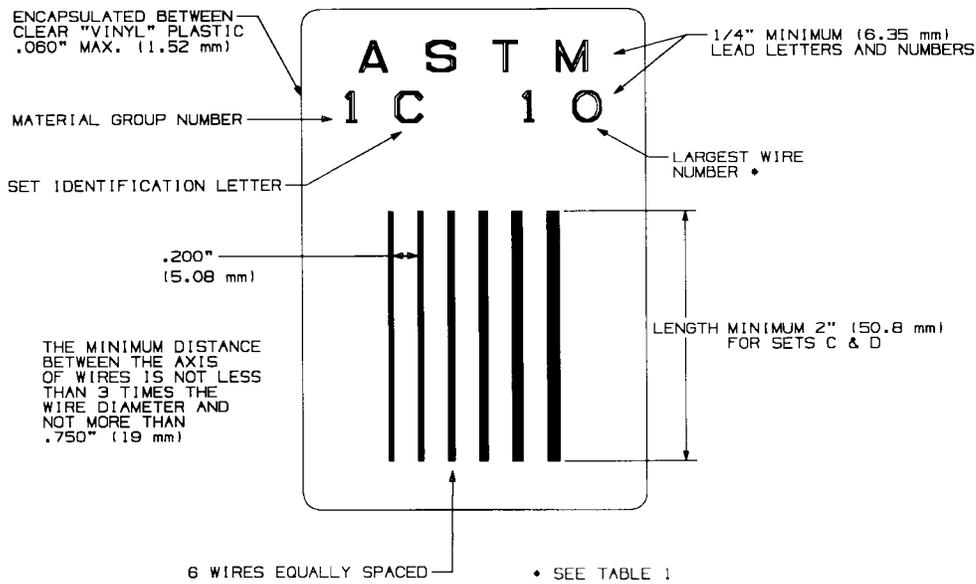


FIG. A1.6 Set C/Alternate 2

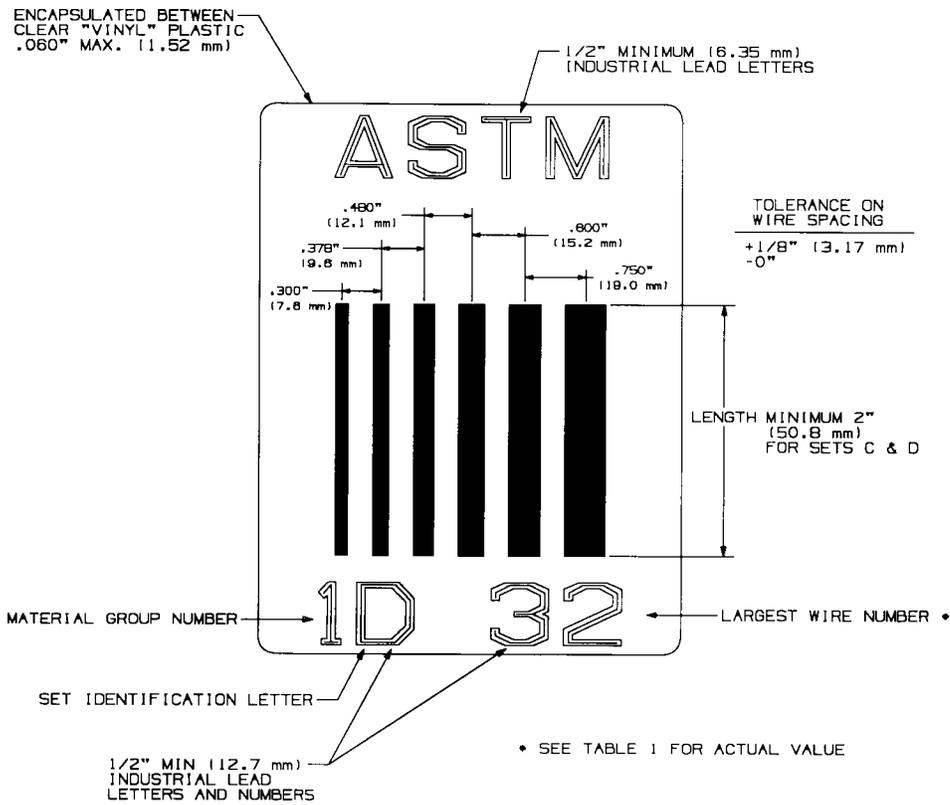


FIG. A1.7 Set D/Alternate 1


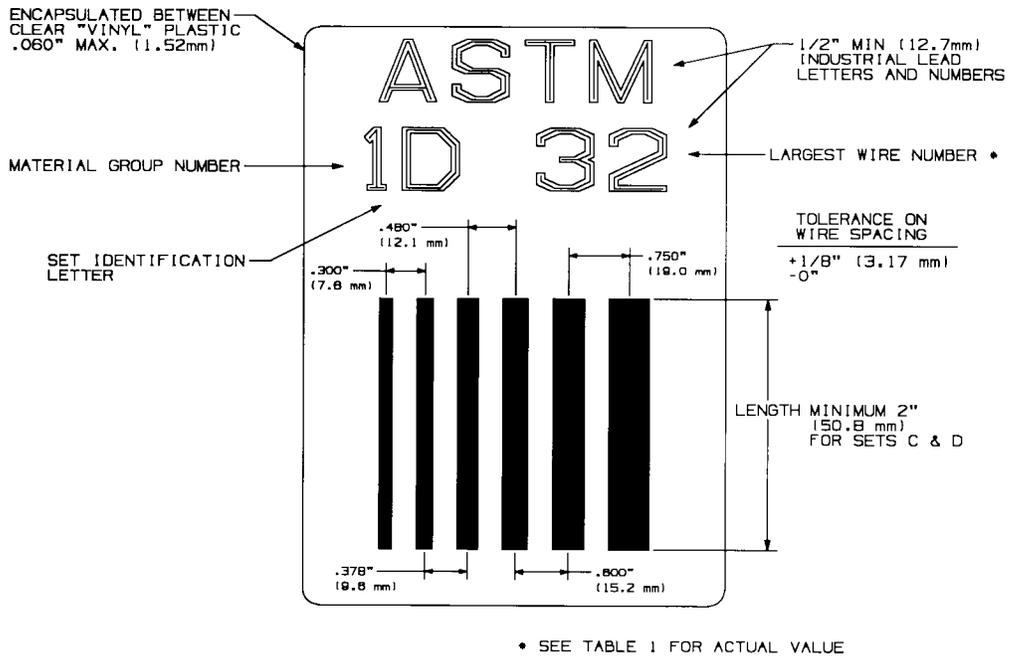


FIG. A1.8 Set D/Alternate 2

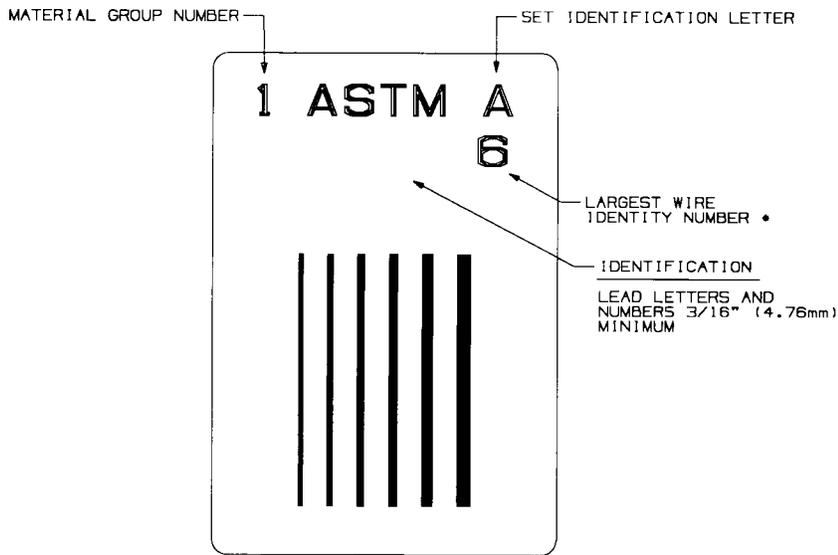

• SEE TABLE 1

NOTE 1—All other IQI requirements as shown on Figs. 1-8 or Figs. A1.1-A1.8 apply.

FIG. A1.9 Alternate Identification Locations and Letter, Number Size-Typical All Sets (A, B, C, D)

TABLE A1.1 Penetrometer Sizes
Wire Diameter in. (mm)

SET A	SET B
0.0032 (0.08) ^A	0.010 (0.25)
0.004 (0.1)	0.013 (0.33)
0.005 (0.13)	0.016 (0.41)
0.0063 (0.16)	0.020 (0.51)
0.008 (0.2)	0.025 (0.64)
0.010 (0.25)	0.032 (0.81)
SET C	SET D
0.032 (0.81)	0.100 (2.5)
0.040 (1.02)	0.126 (3.2)
0.050 (1.27)	0.160 (4.06)
0.063 (1.6)	0.20 (5.1)
0.080 (2.03)	0.25 (6.4)
0.100 (2.5)	0.32 (0.81)

^A The 0.0032 wire may be used to establish a special quality level as agreed upon between the purchaser and the supplier.

APPENDIX

(Nonmandatory Information)

X1. CALCULATING OTHER EQUIVALENTS

X1.1 The equation to determine the equivalencies between wire and (hole type) IQI's is as follows:

$$F^3 d^3 l = T^2 H^2 (\pi/4)$$

where:

- F = form factor for wire, 0.79,
- d = wire diameter, in. (mm),
- l = effective length of wire, 0.3 in. (7.6 mm),
- T = plaque thickness, in. (mm), and

H = diameter of hole, in. (mm).

X1.2 It should be noted that the wire and plaque (hole type) IQI sensitivities cannot be related by a fixed constant.

X1.3 Figs. X1.1 and X1.2 are conversion charts for hole type IQI's containing 1T and 2T holes to wires. The sensitivities are given as a percentage of the specimen thickness.

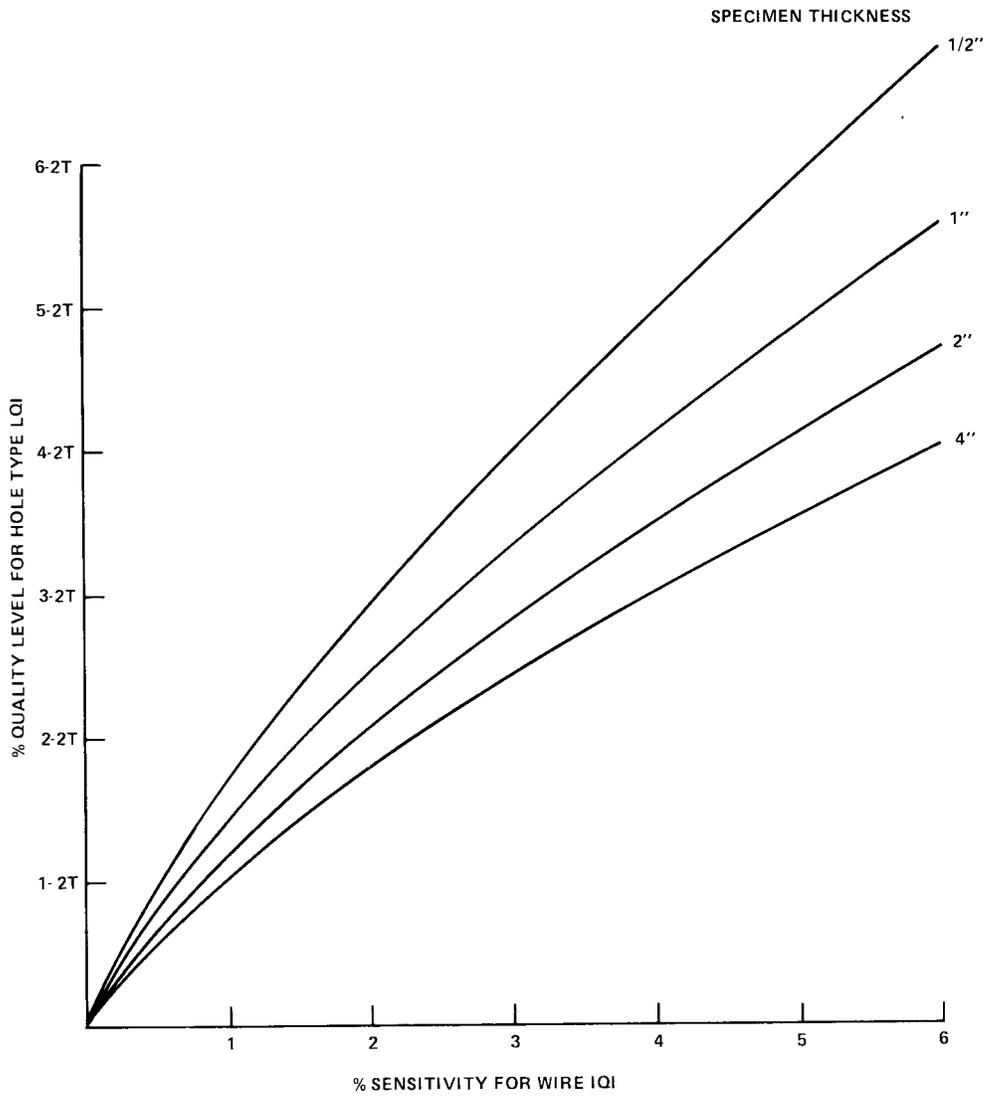


FIG. X1.1 Conversion Chart for 2-T Quality Level Holes to % Wire Sensitivity

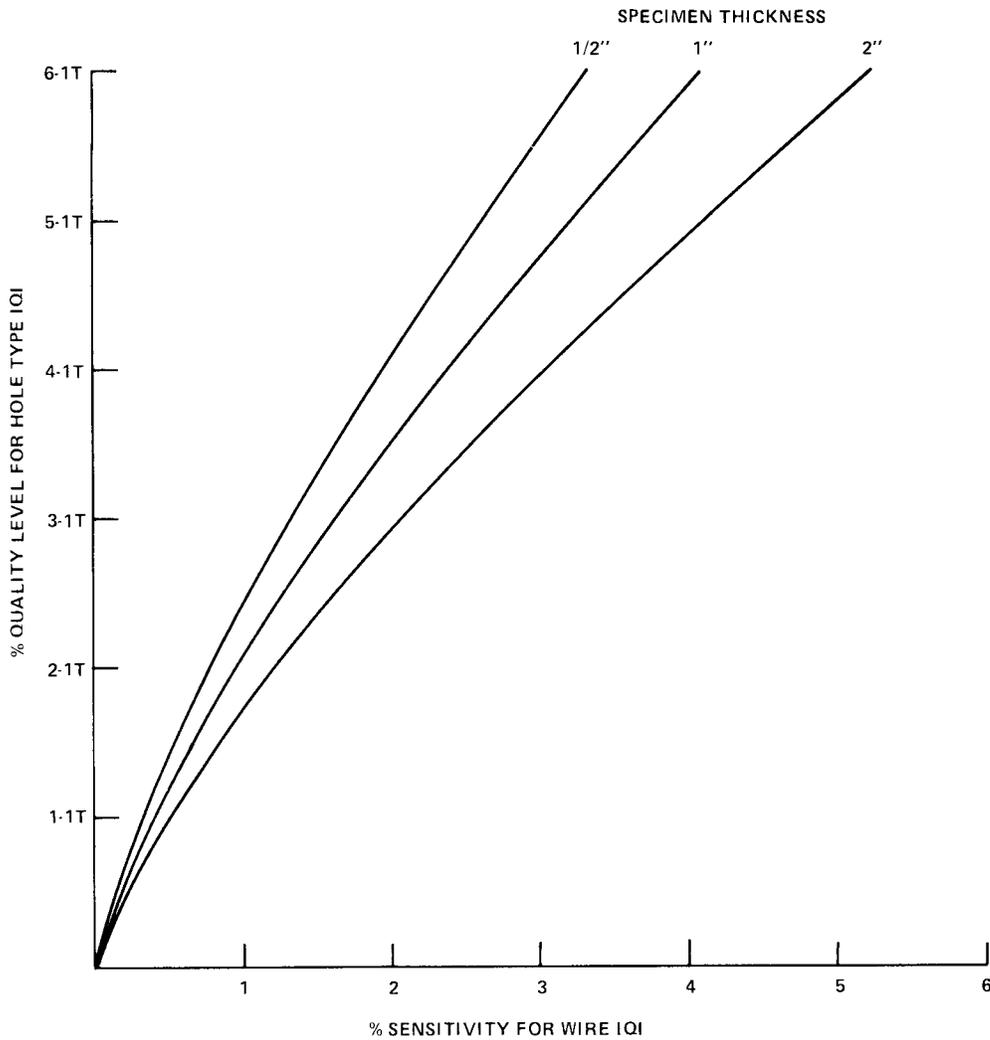


FIG. X1.2 Conversion Chart for 1-T Quality Level Holes to % Wire Sensitivity

The American Society for Testing and Materials takes no position respecting the validity of any patent rights asserted in connection with any item mentioned in this standard. Users of this standard are expressly advised that determination of the validity of any such patent rights, and the risk of infringement of such rights, are entirely their own responsibility.

This standard is subject to revision at any time by the responsible technical committee and must be reviewed every five years and if not revised, either reapproved or withdrawn. Your comments are invited either for revision of this standard or for additional standards and should be addressed to ASTM Headquarters. Your comments will receive careful consideration at a meeting of the responsible technical committee, which you may attend. If you feel that your comments have not received a fair hearing you should make your views known to the ASTM Committee on Standards, 100 Barr Harbor Drive, West Conshohocken, PA 19428.

This standard is copyrighted by ASTM, 100 Barr Harbor Drive, West Conshohocken, PA 19428-2959, United States. Individual reprints (single or multiple copies) of this standard may be obtained by contacting ASTM at the above address or at 610-832-9585 (phone), 610-832-9555 (fax), or service@astm.org (e-mail); or through the ASTM website (<http://www.astm.org>).